

FIGURE 1

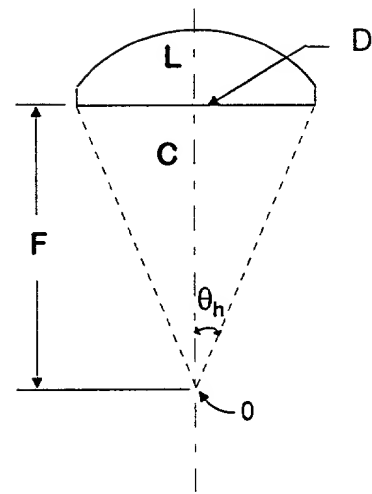


FIGURE 2

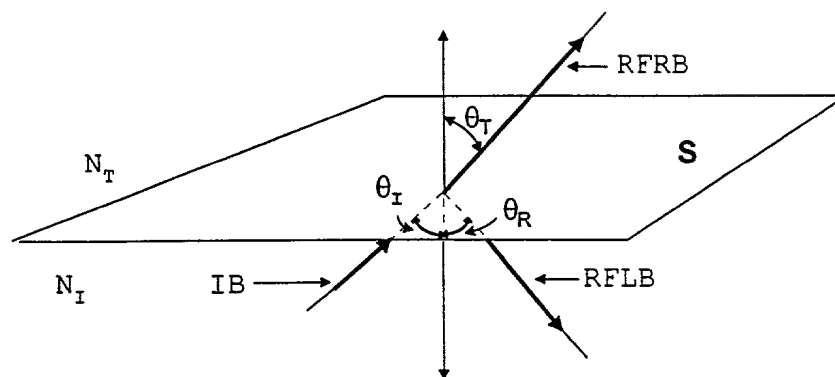


FIGURE 3

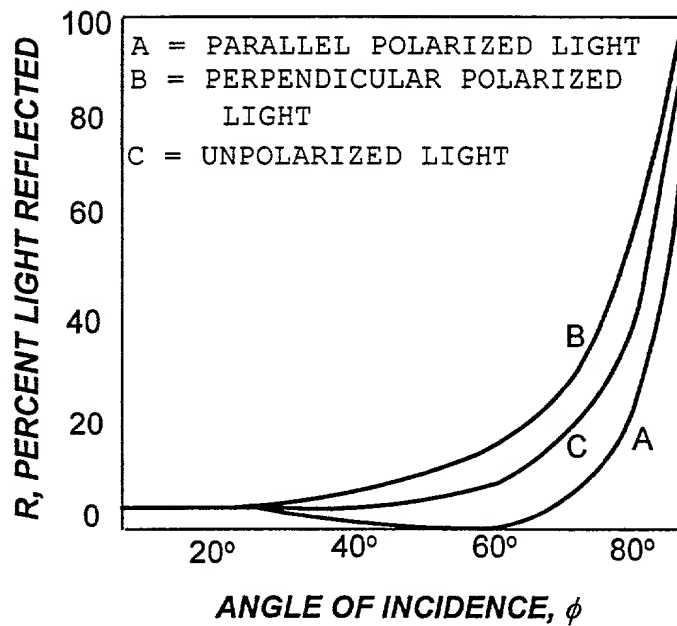


FIGURE 4A

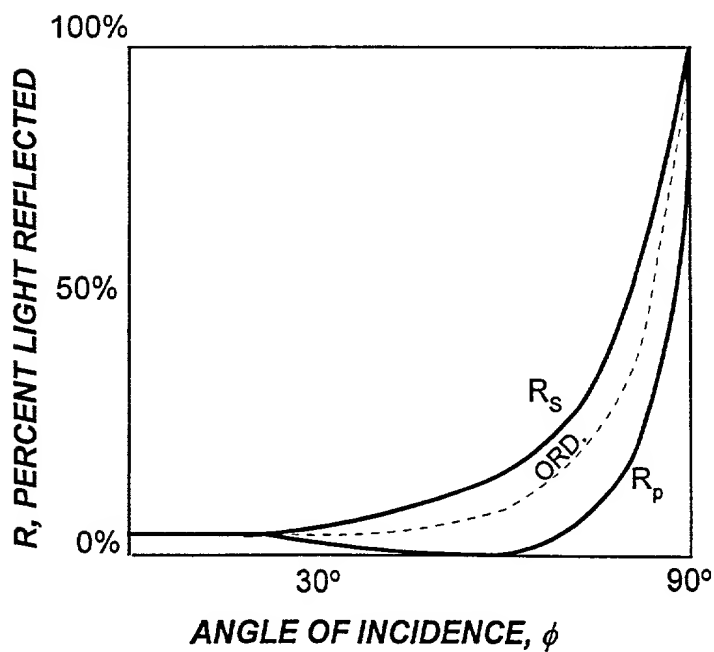


FIGURE 4B

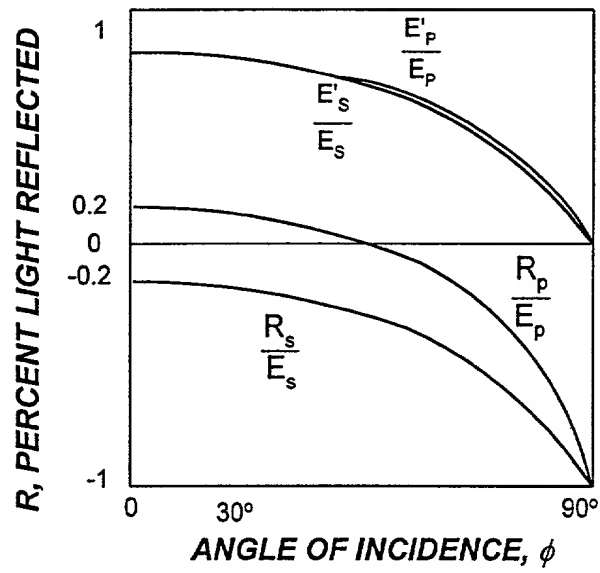


FIGURE 4C

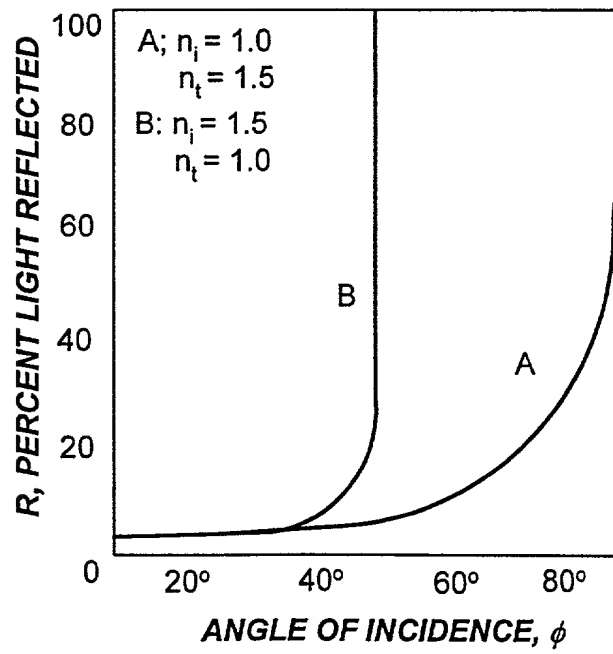


FIGURE 5A

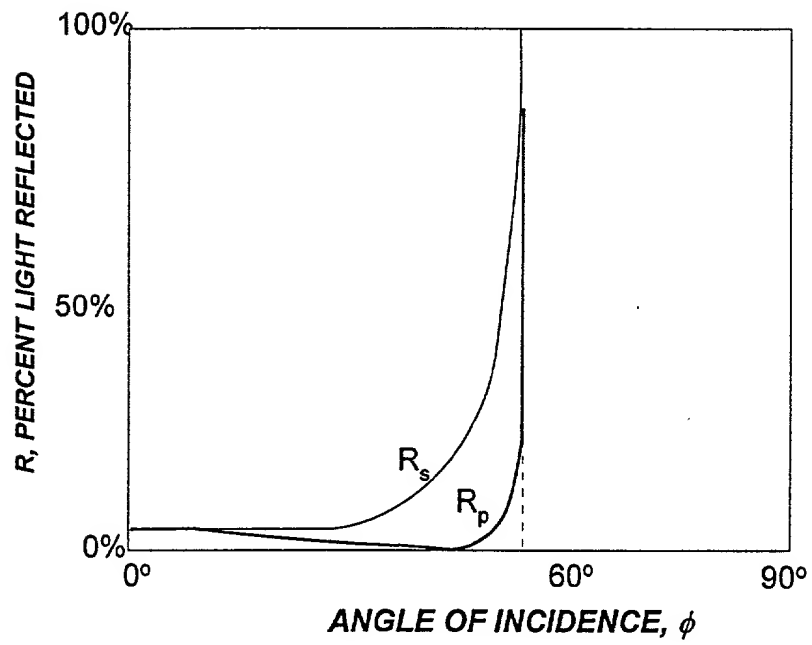


FIGURE 5B

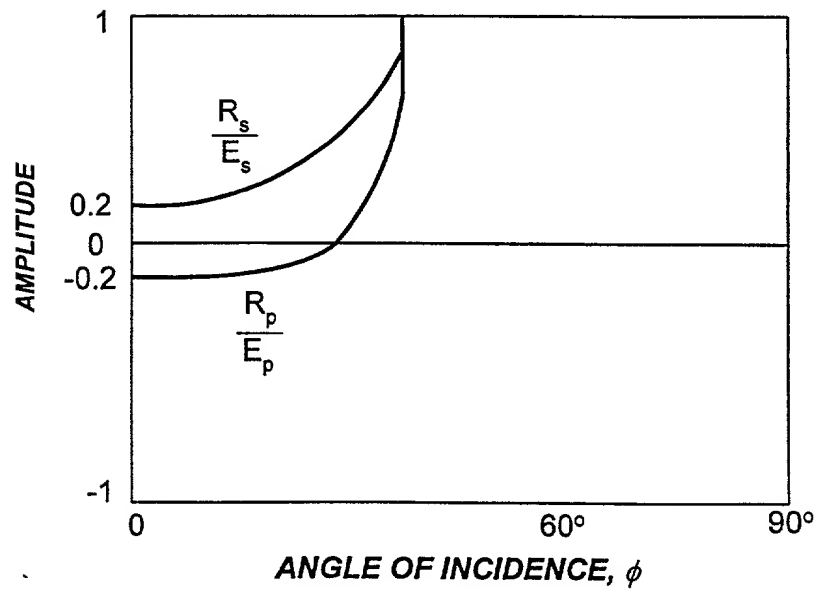


FIGURE 5C

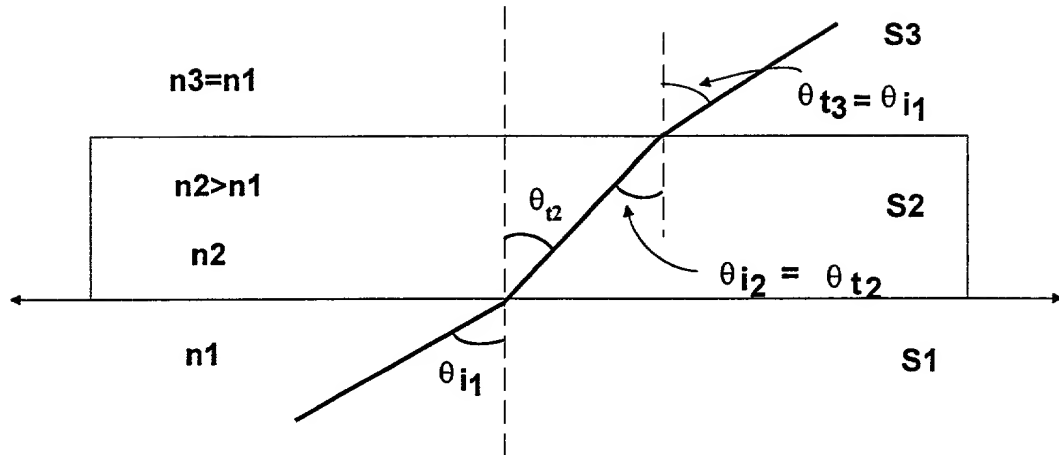


FIGURE 6

$n_i = 1$        $n_t = 1.5$

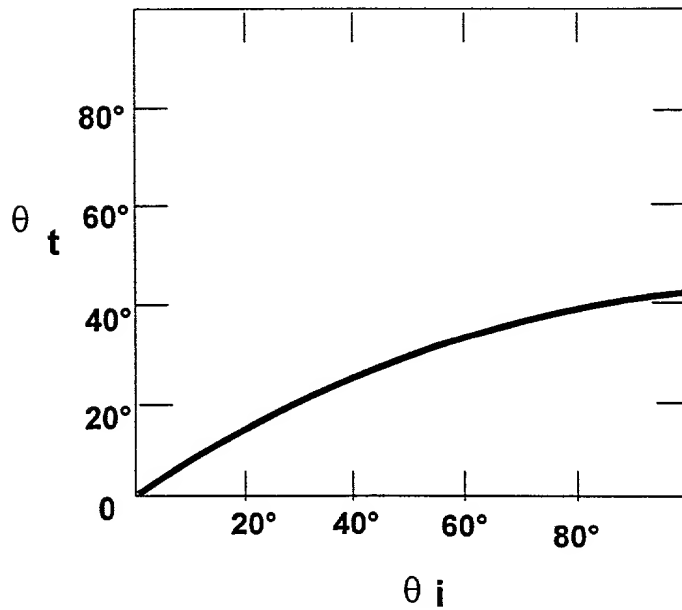


FIGURE 7

6/30

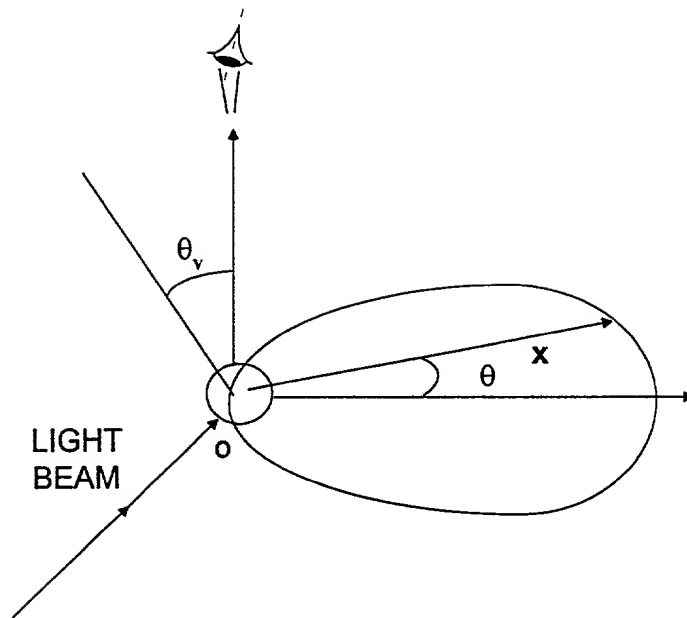


FIGURE 8

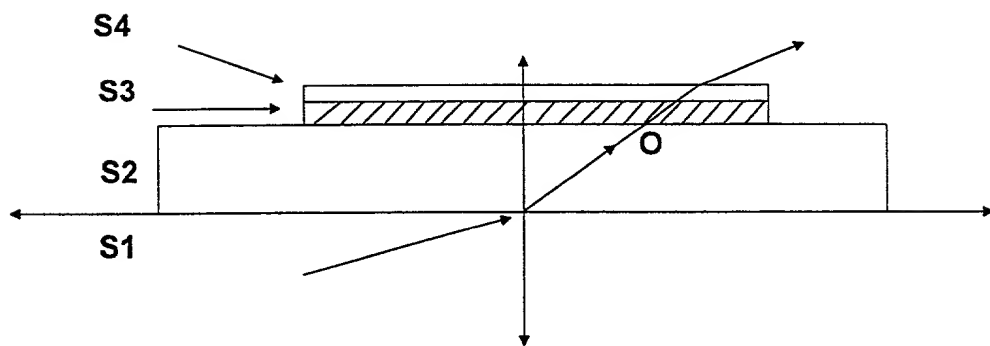


FIGURE 9

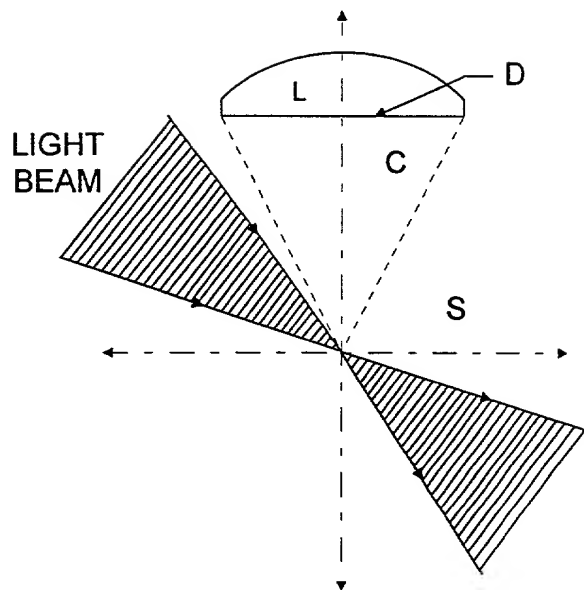


FIGURE 10

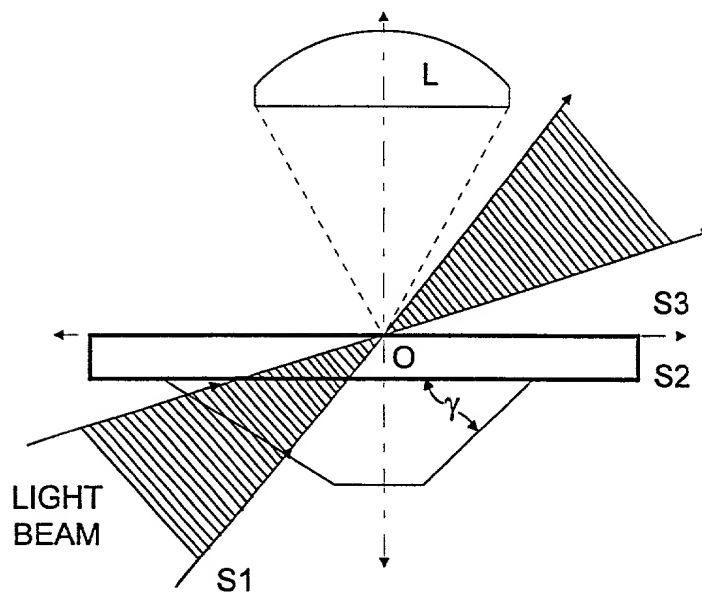


FIGURE 11

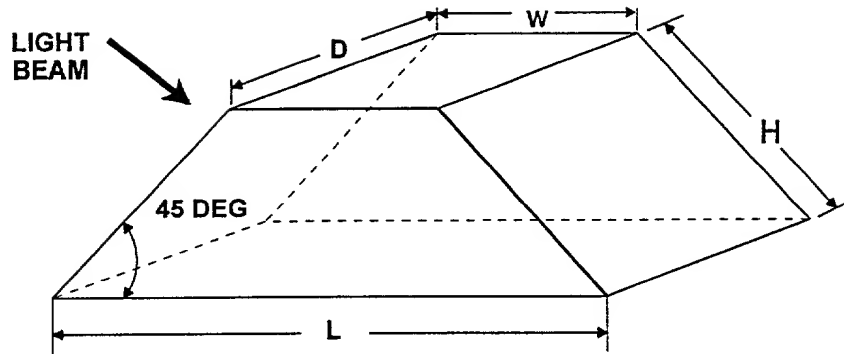


FIGURE 12A

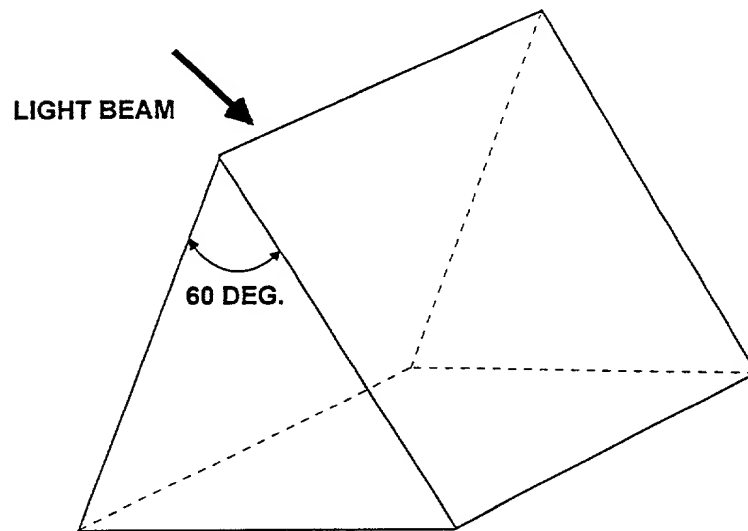


FIGURE 12B

Downloaded from www.ascelibrary.org



9/30

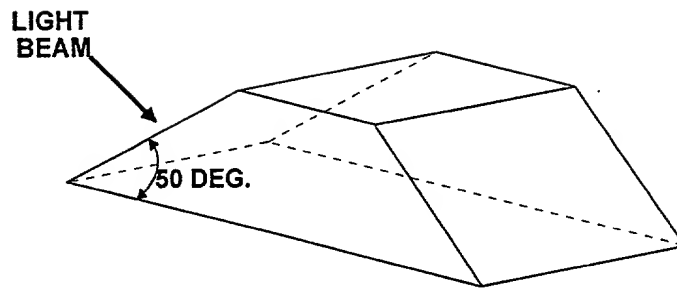


FIGURE 12C


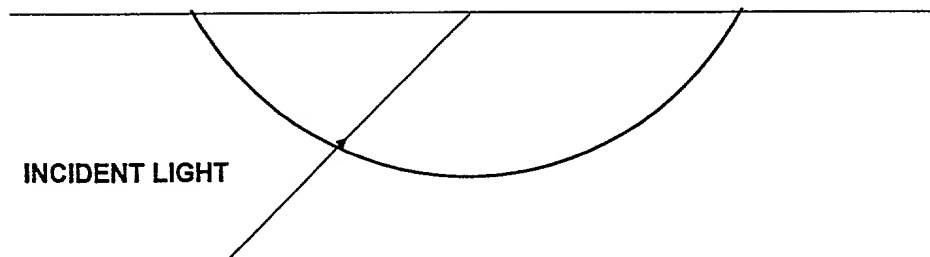


FIGURE 12D

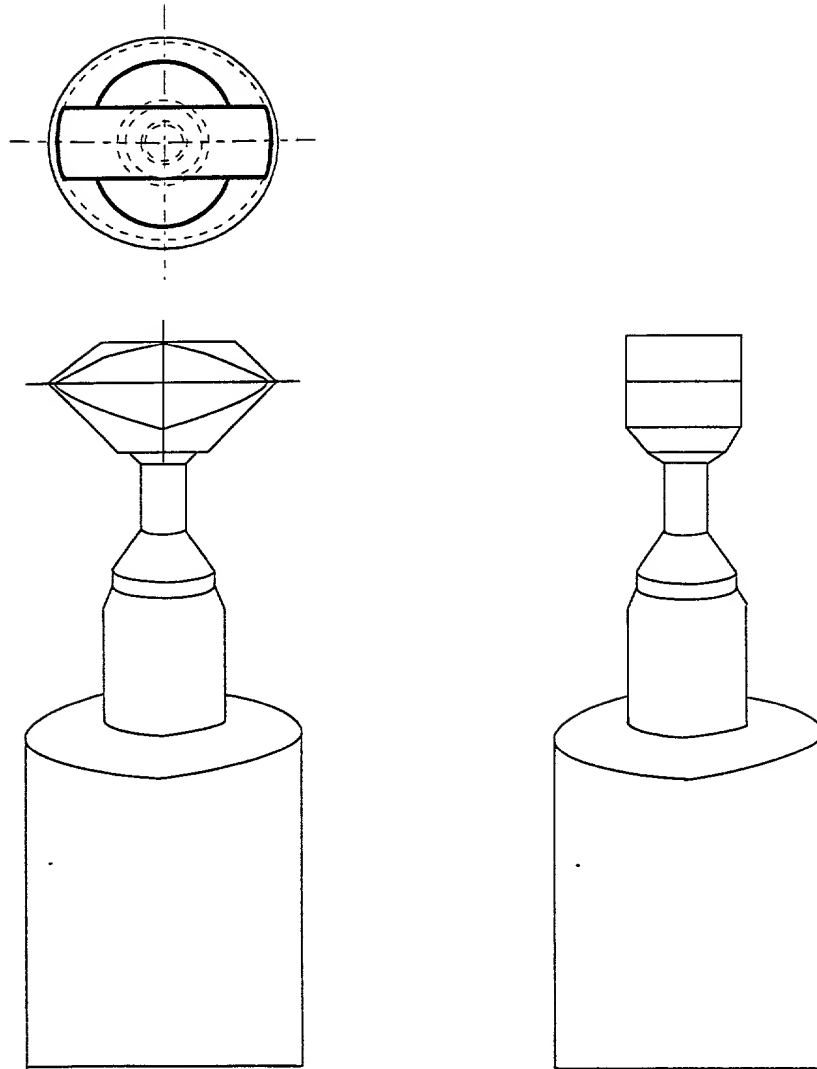

NOT TO SCALE

**FIGURE 12E**

11/30

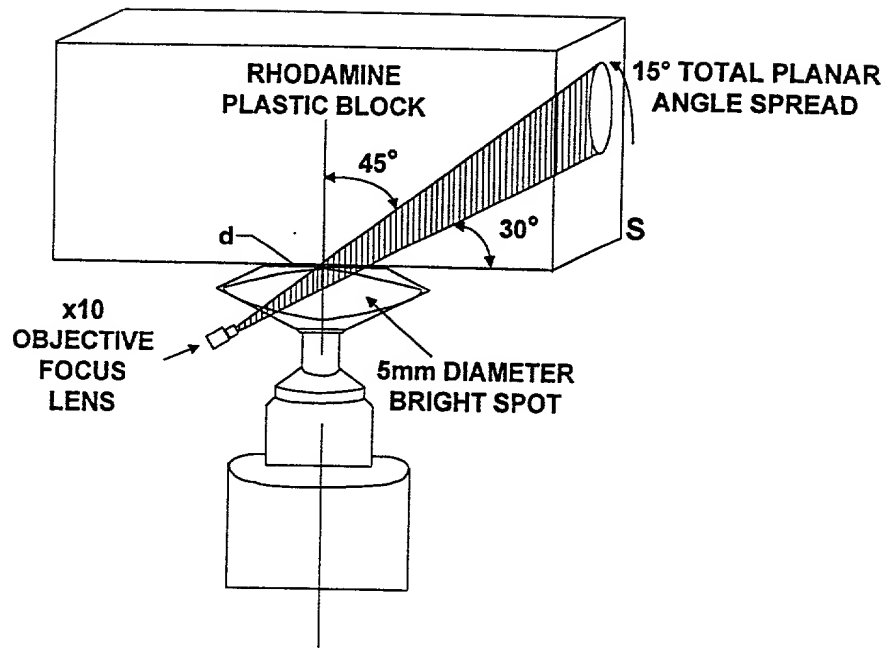


FIGURE 13

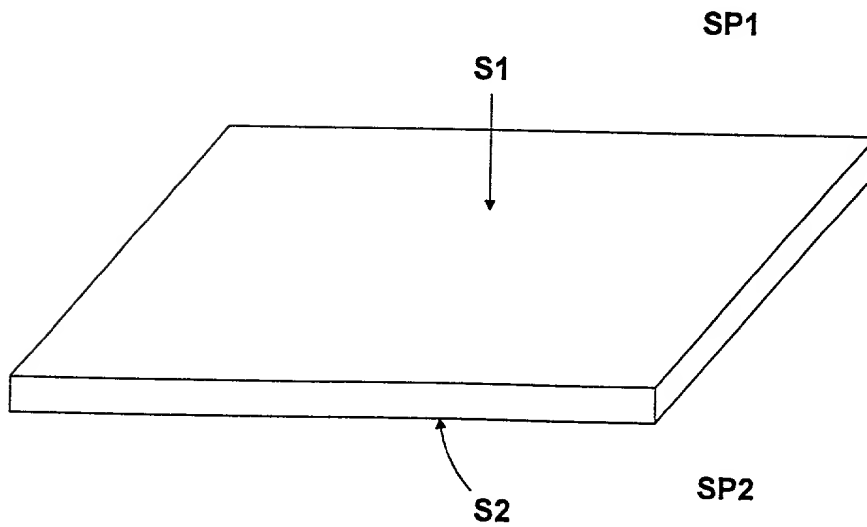


FIGURE 14

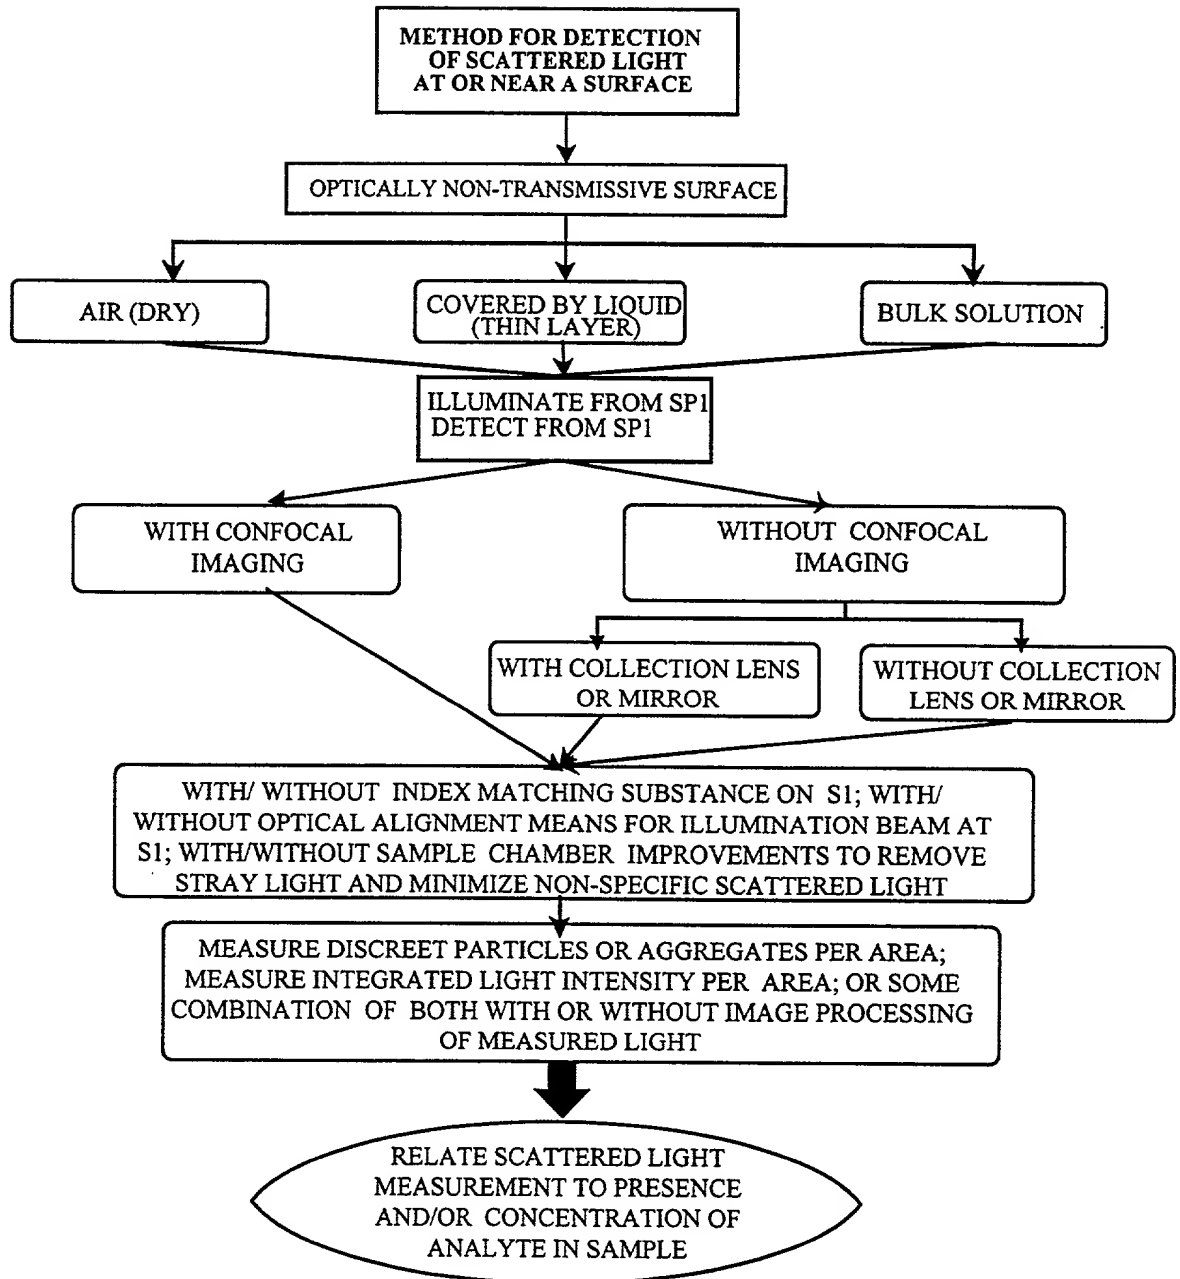


FIGURE 15A

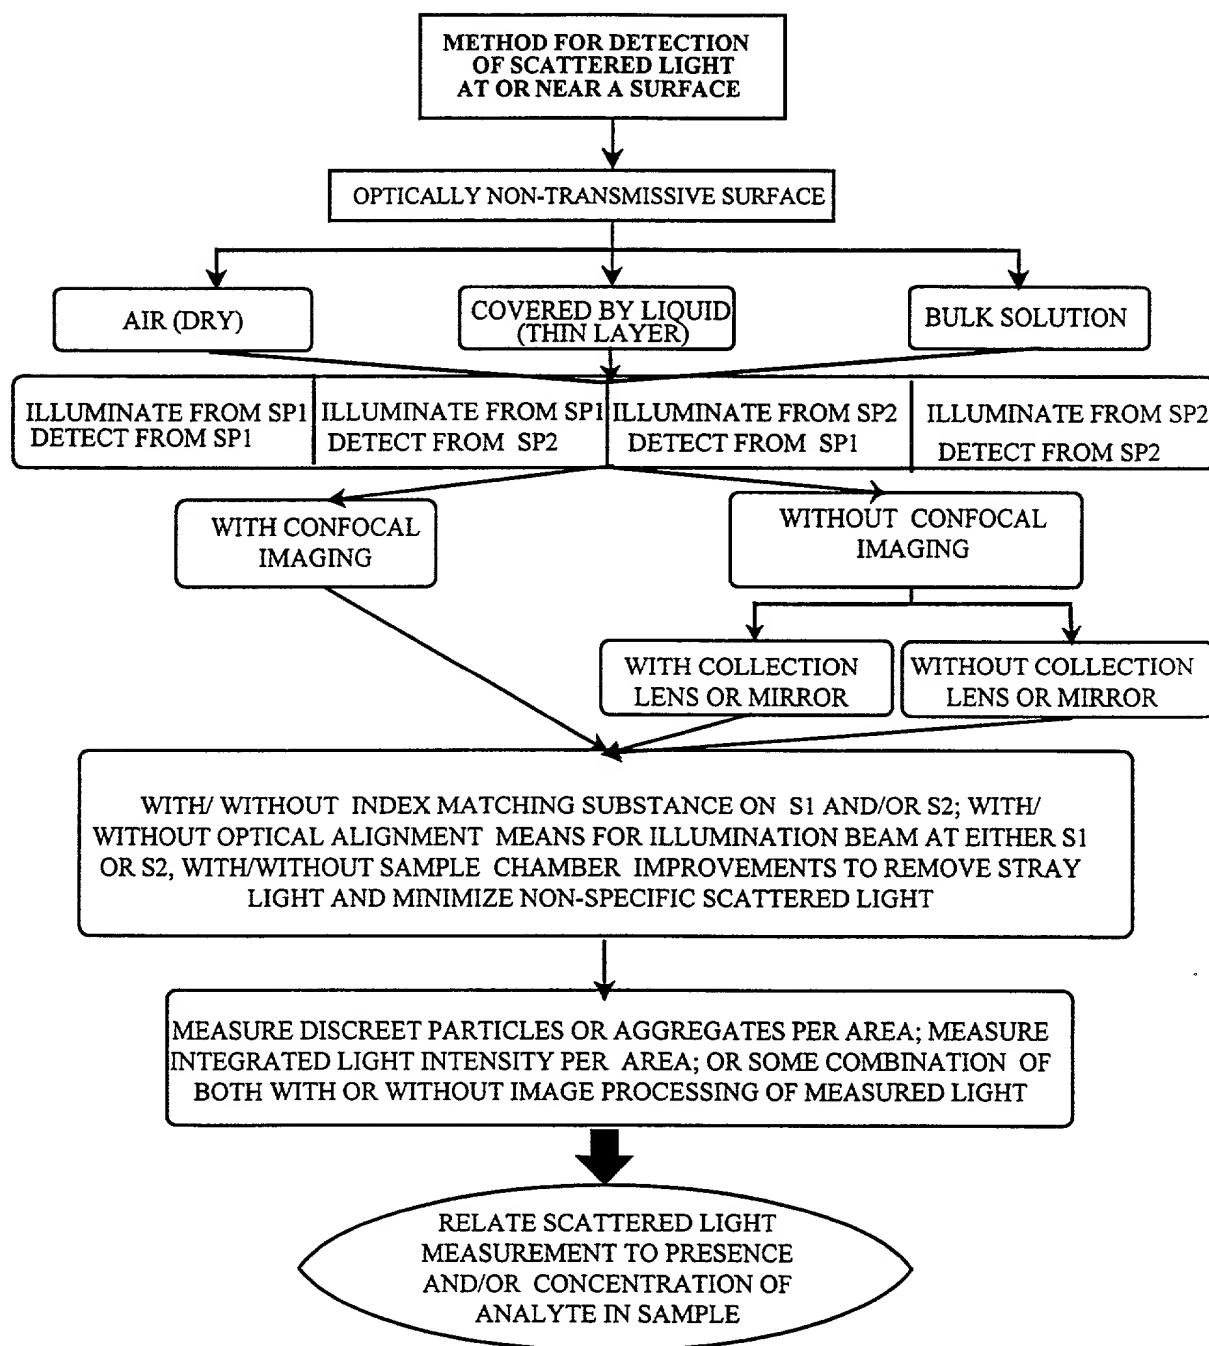


FIGURE 15B

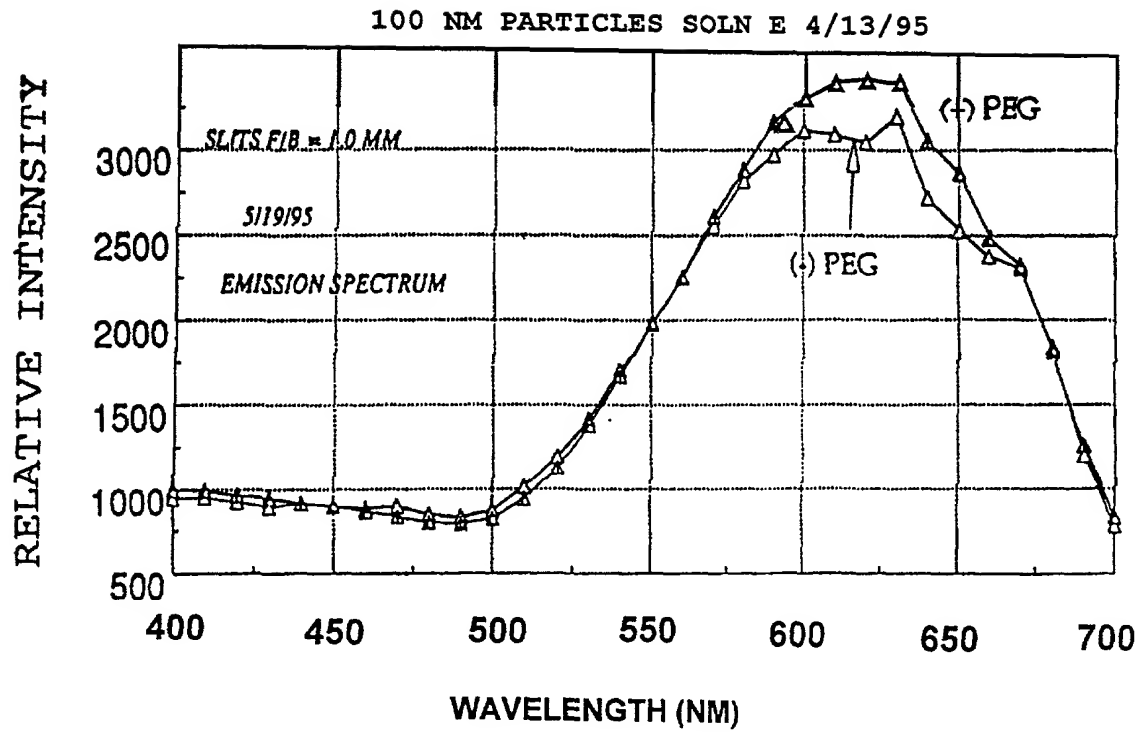


FIGURE 16



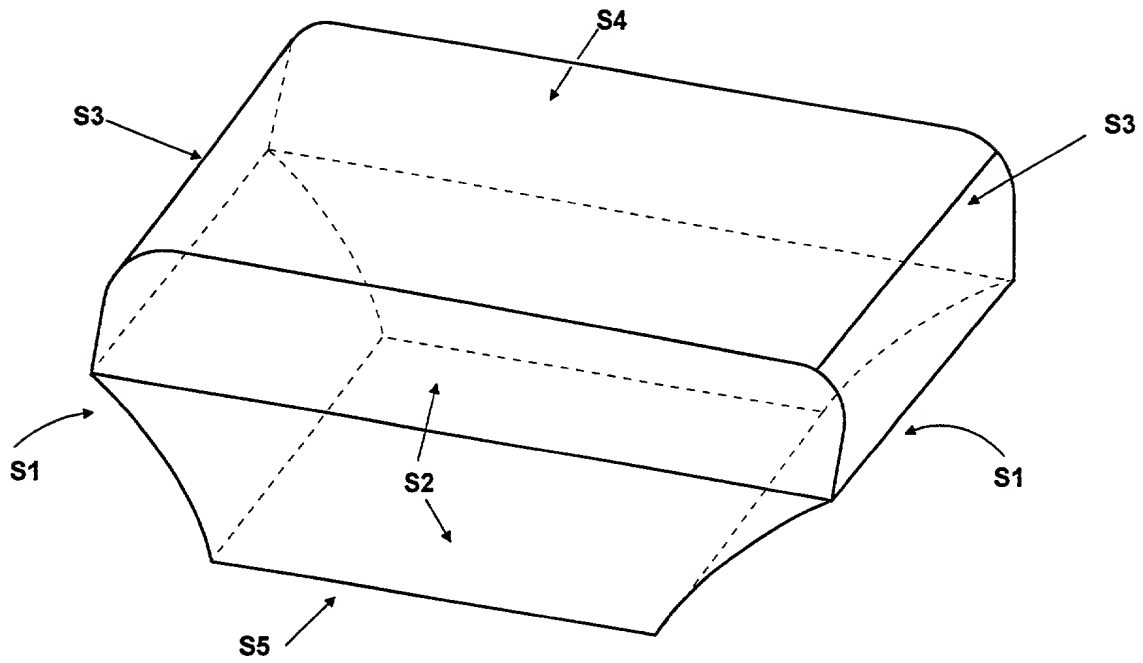


FIGURE 19

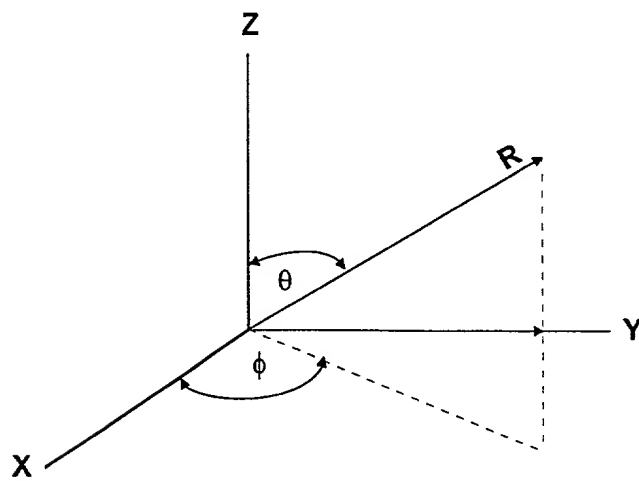


FIGURE 20



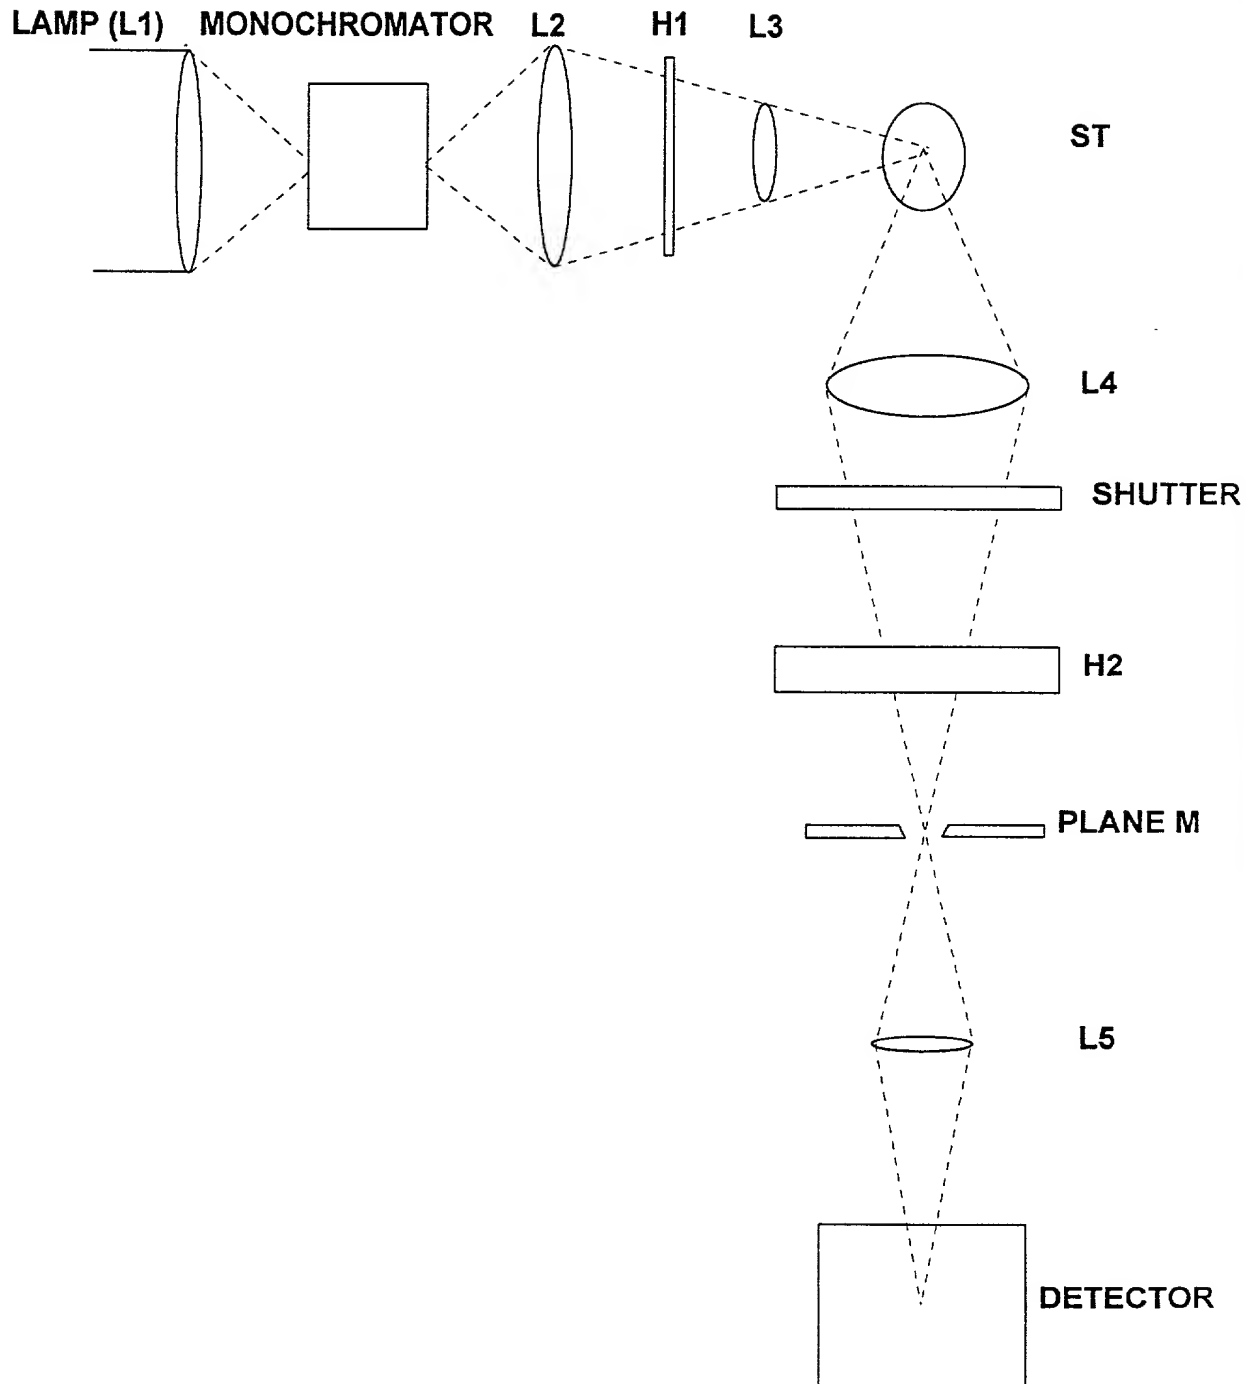


FIGURE 21

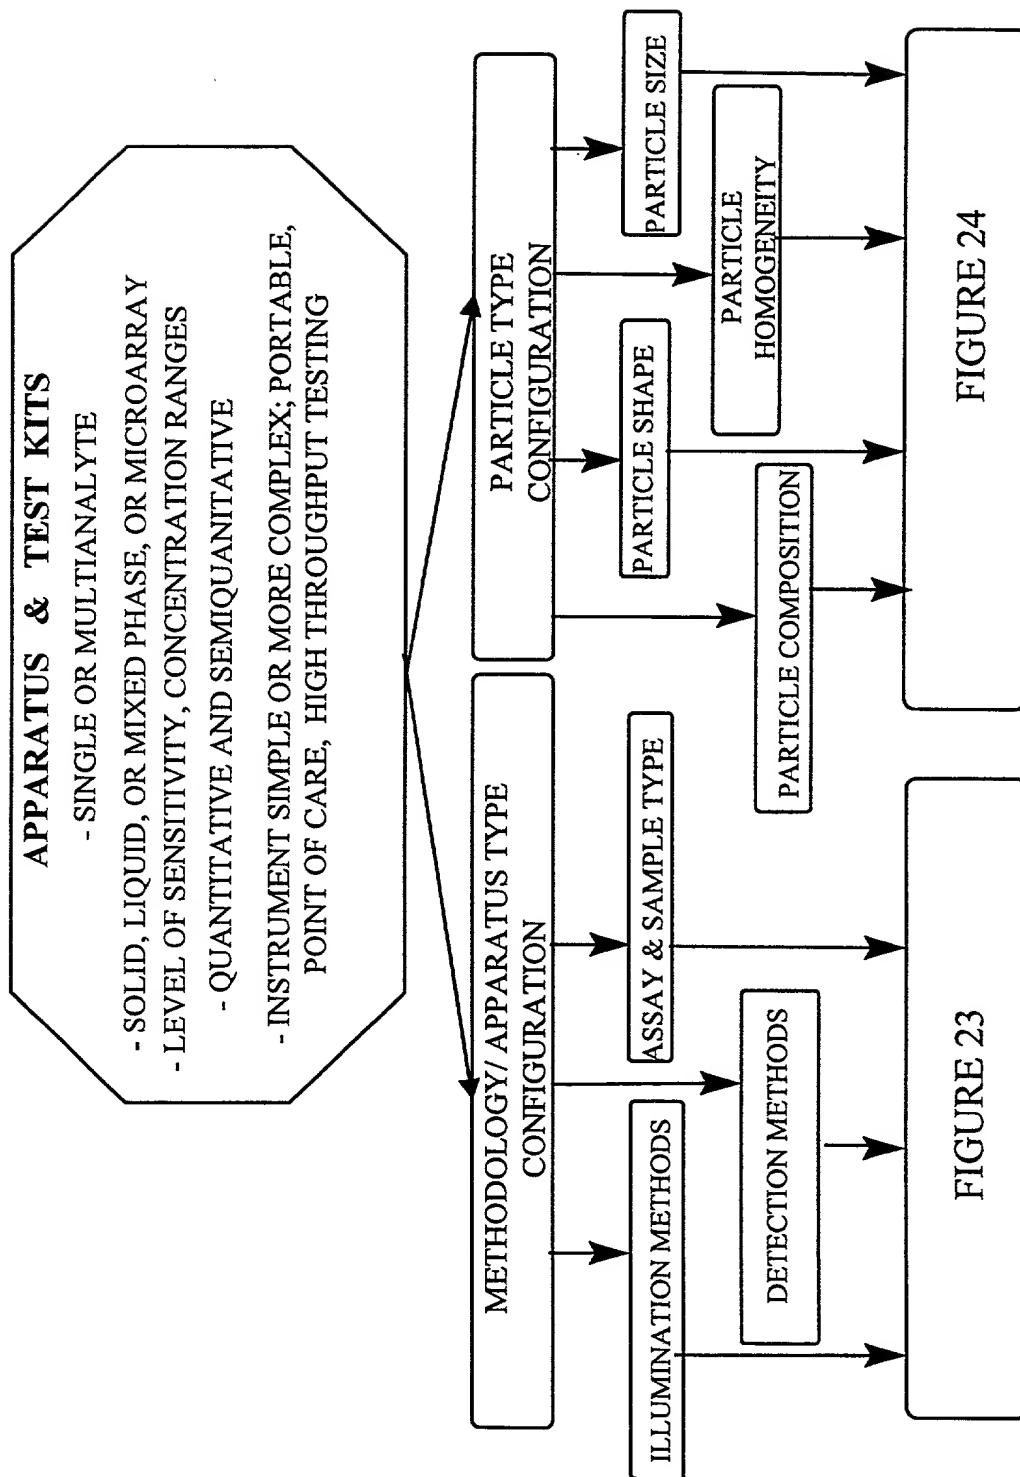


FIGURE 22

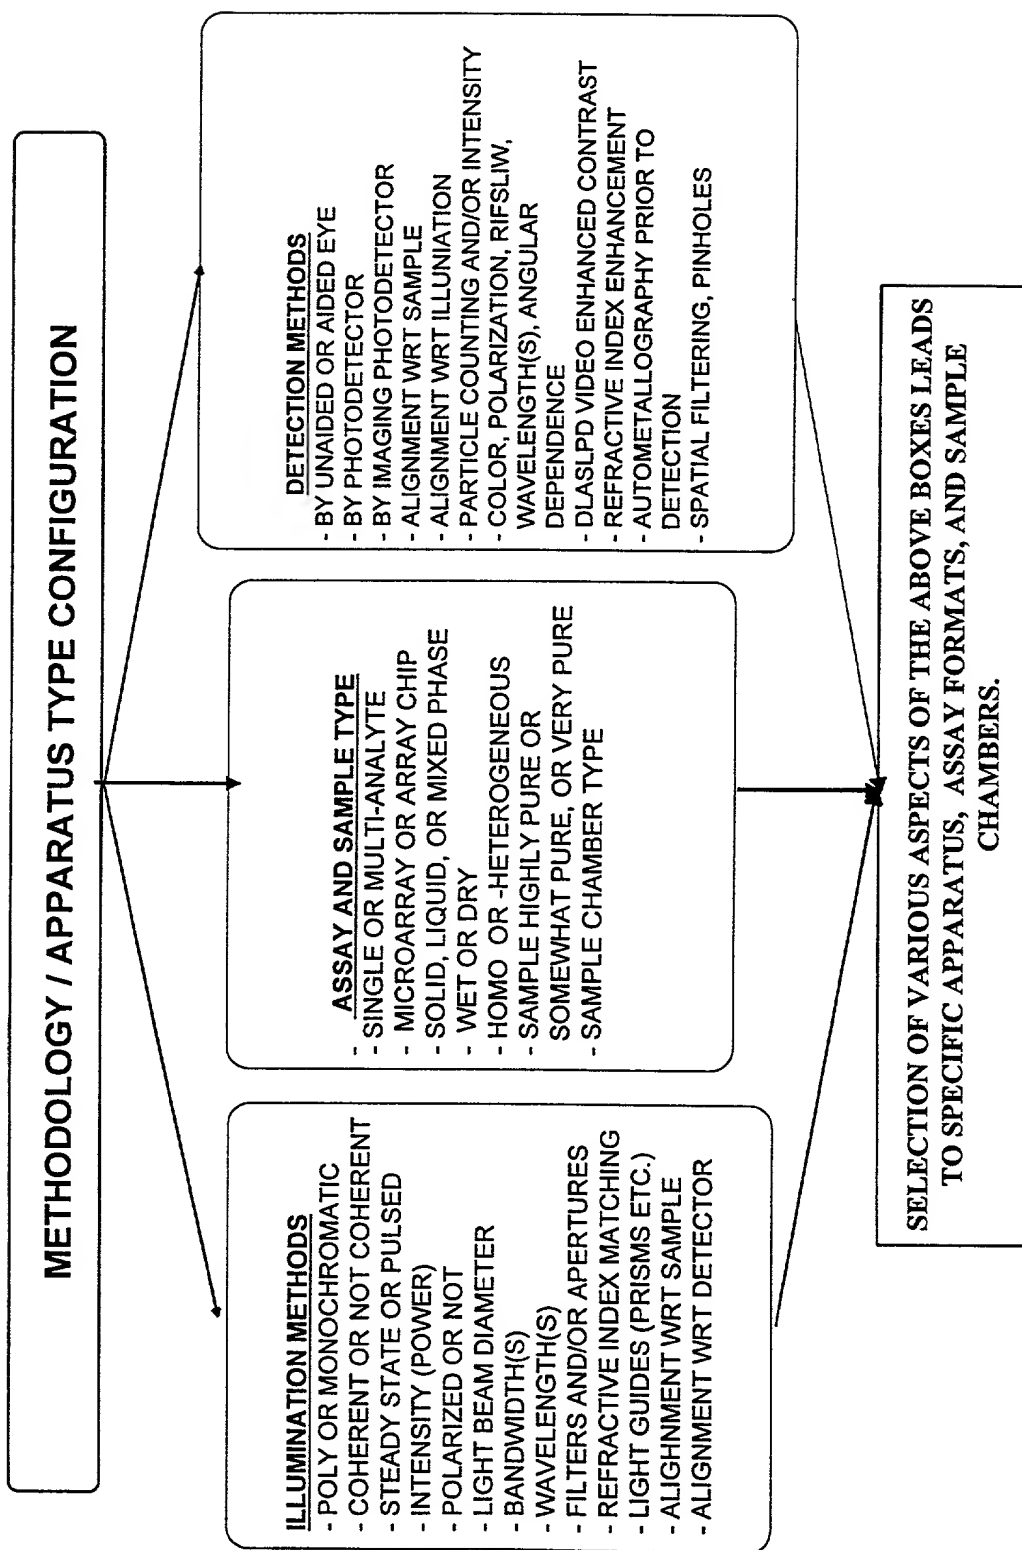


FIGURE 23

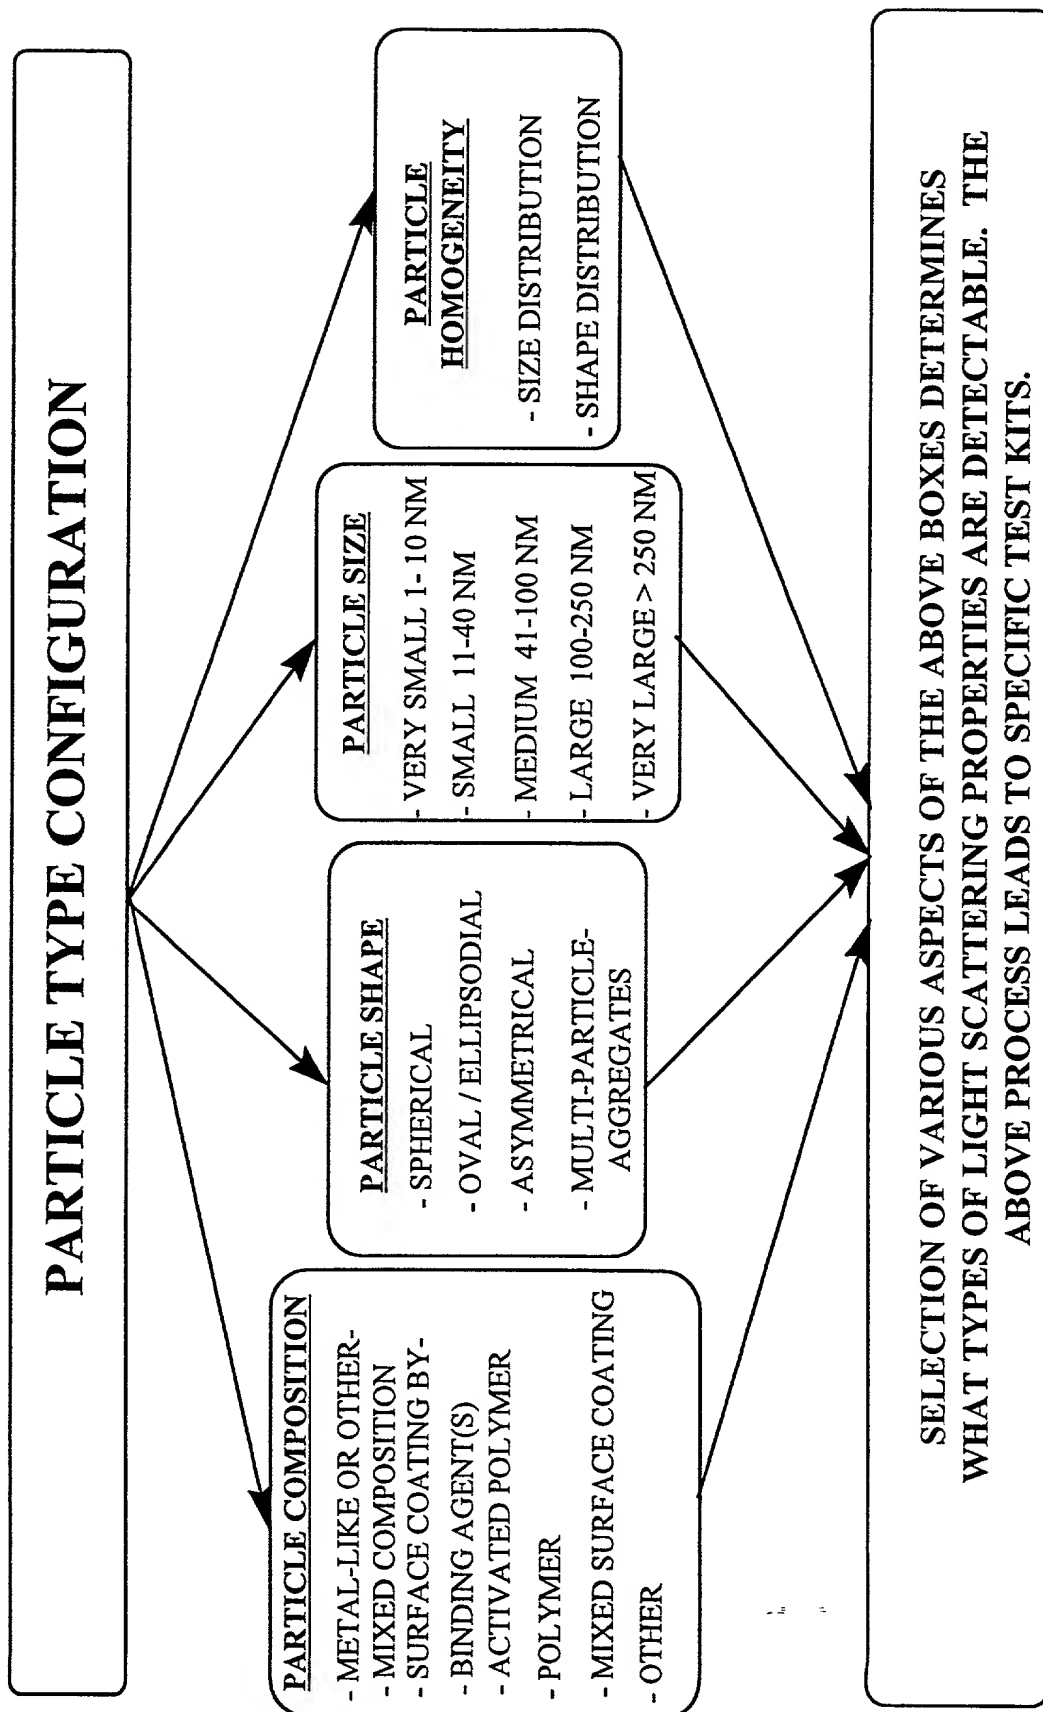
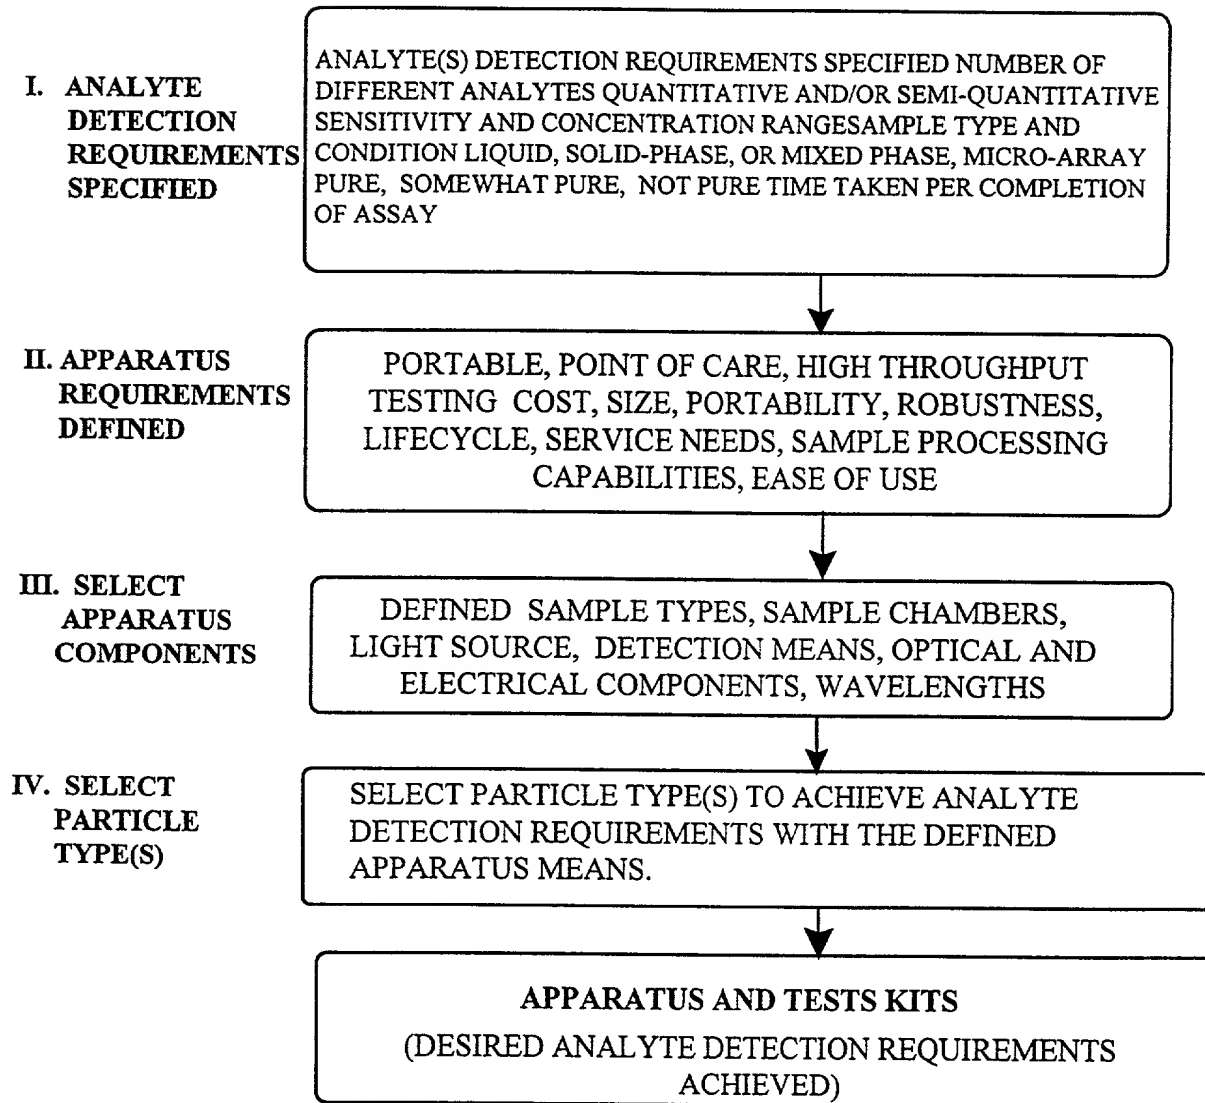
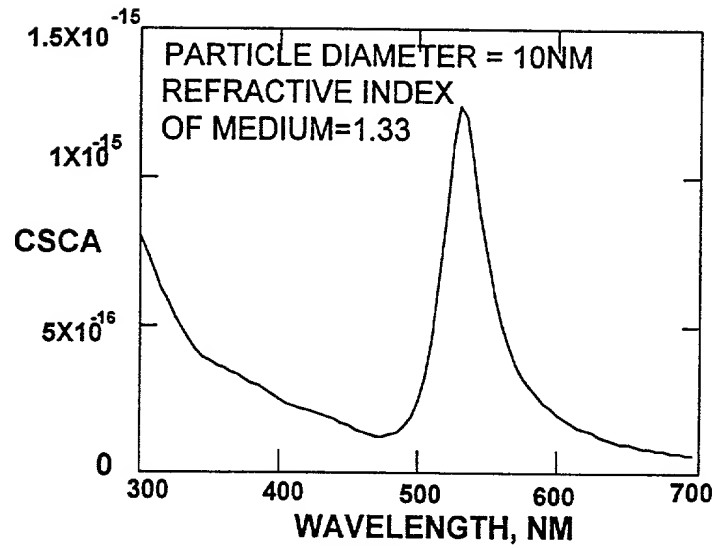
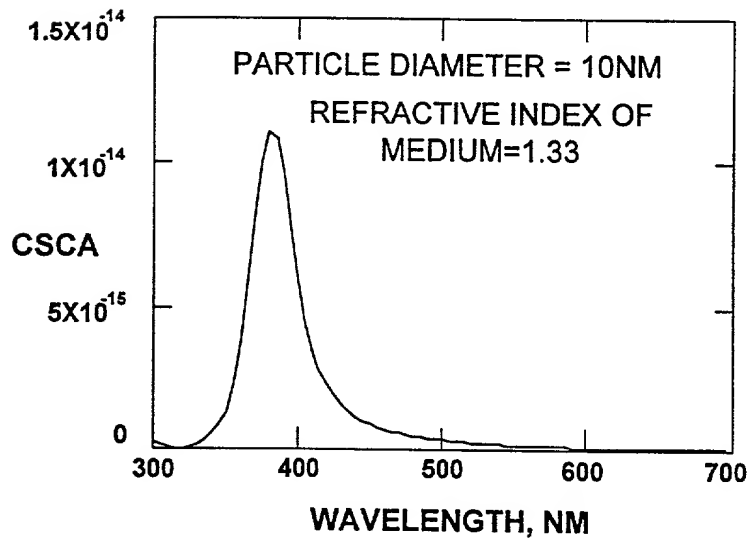




FIGURE 24



**PRACTICE OF INVENTION  
TO A SPECIFIC DIAGNOSTIC NEED  
LEADING TO SPECIFIC APPARATUS AND  
TEST KITS**



**FIGURE 25**

**GOLD****FIGURE 26A****SILVER****FIGURE 26B**

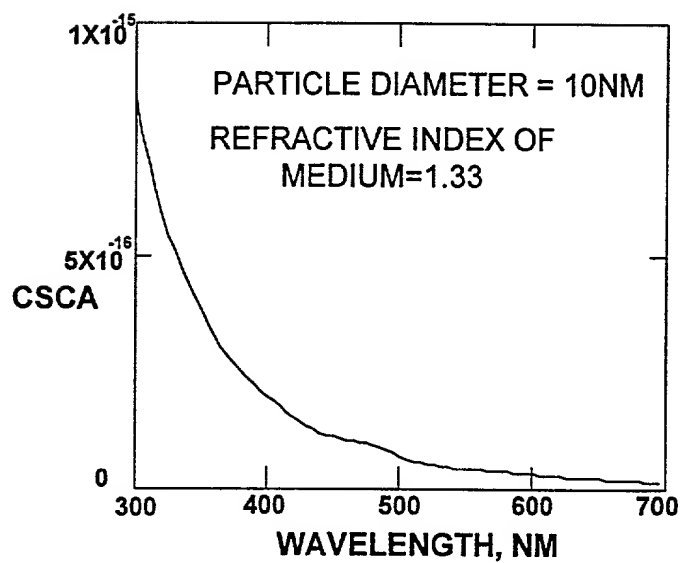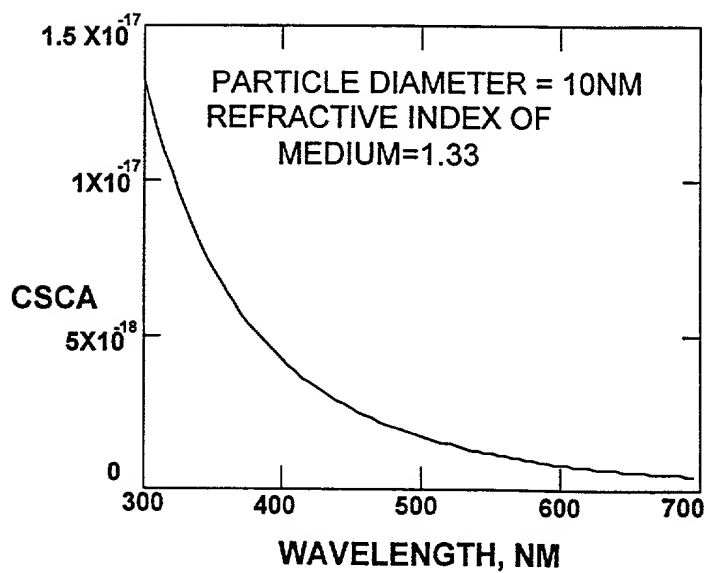**SELENIUM****FIGURE 26C****POLYSTYRENE****FIGURE 26D**

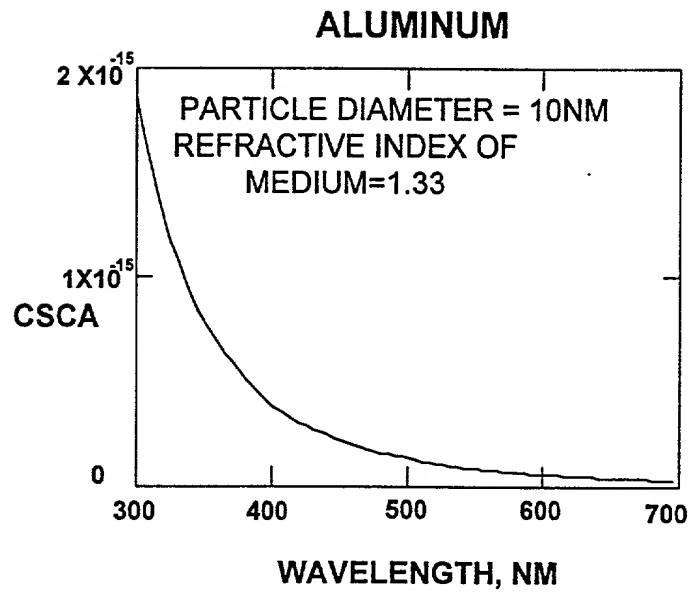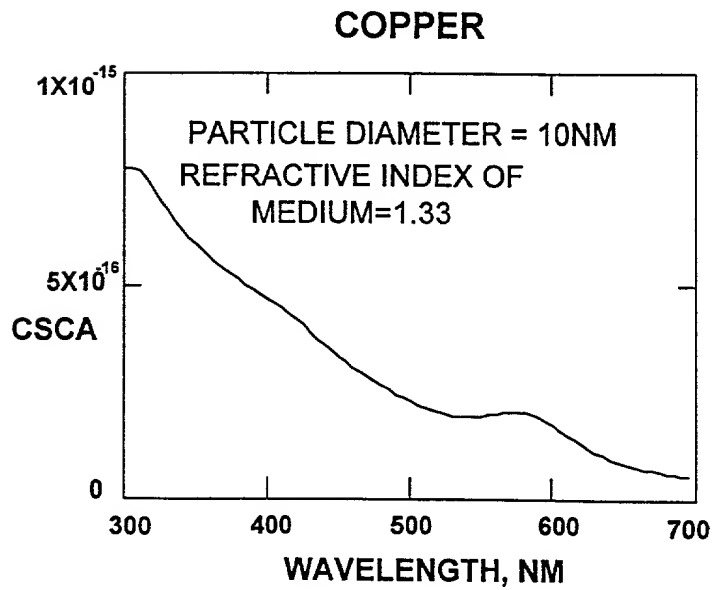**FIGURE 26E****FIGURE 26F**



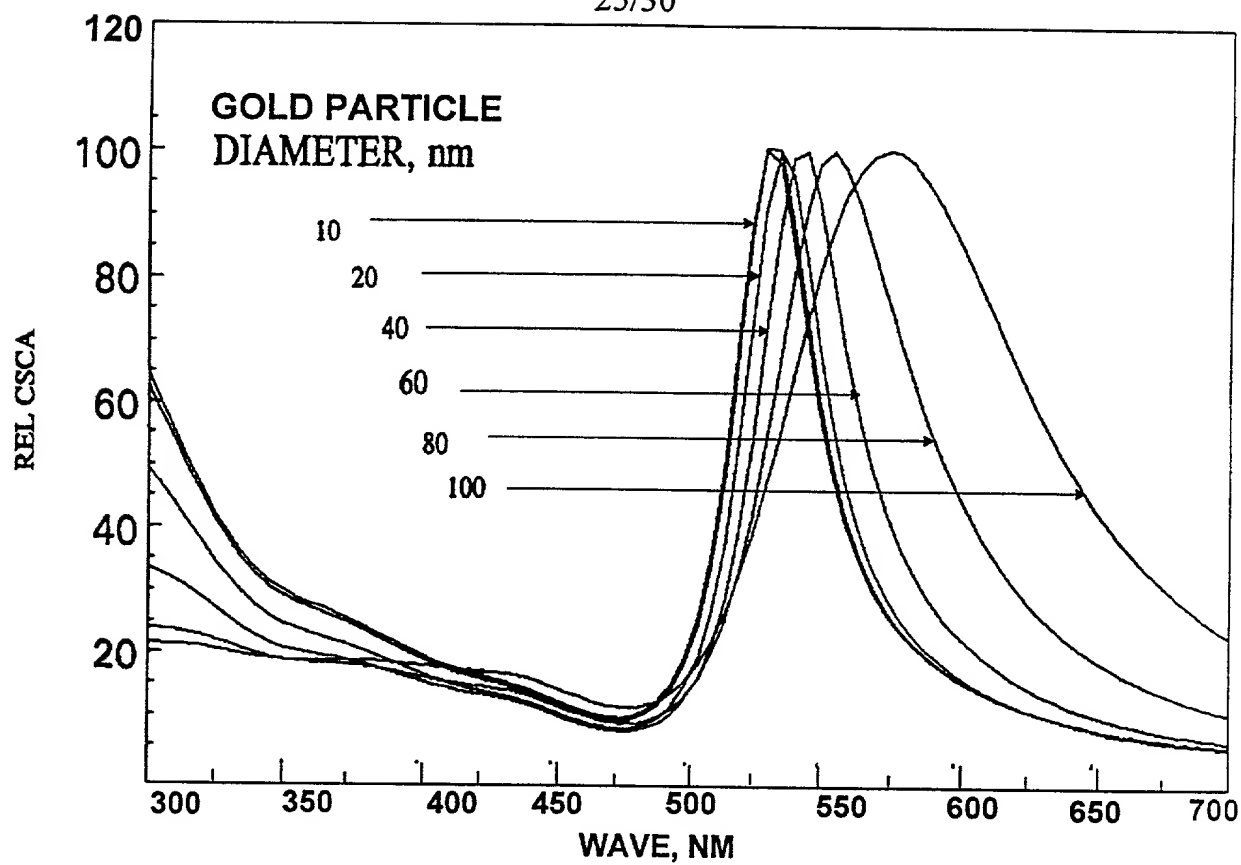


FIGURE 27

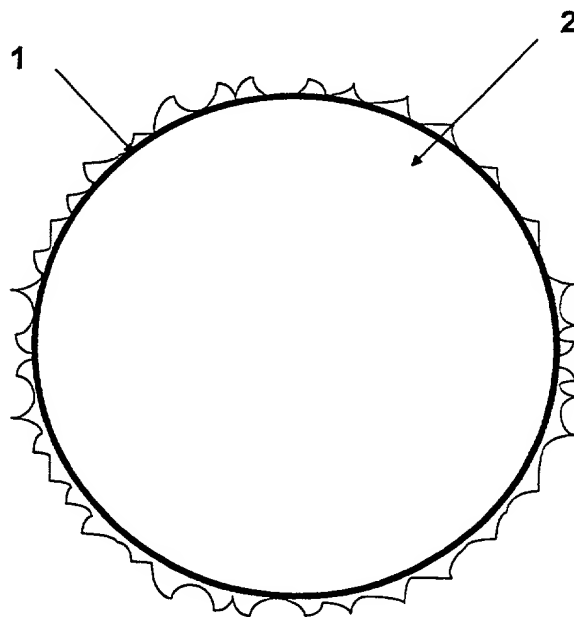


FIGURE 28

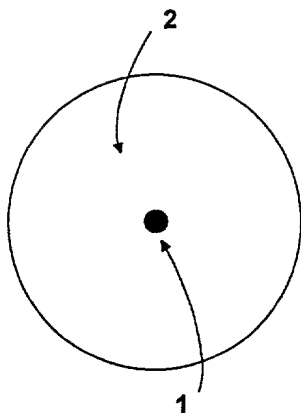


FIGURE 29A

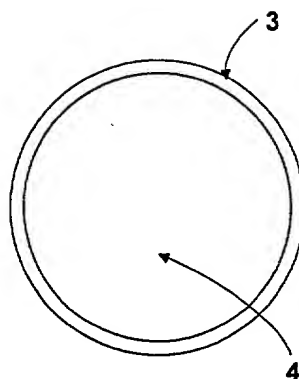


FIGURE 29B

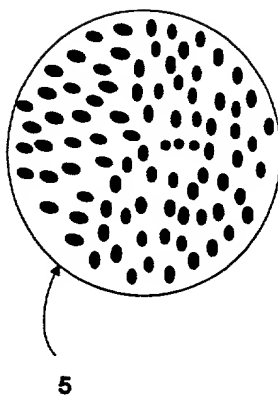


FIGURE 29C



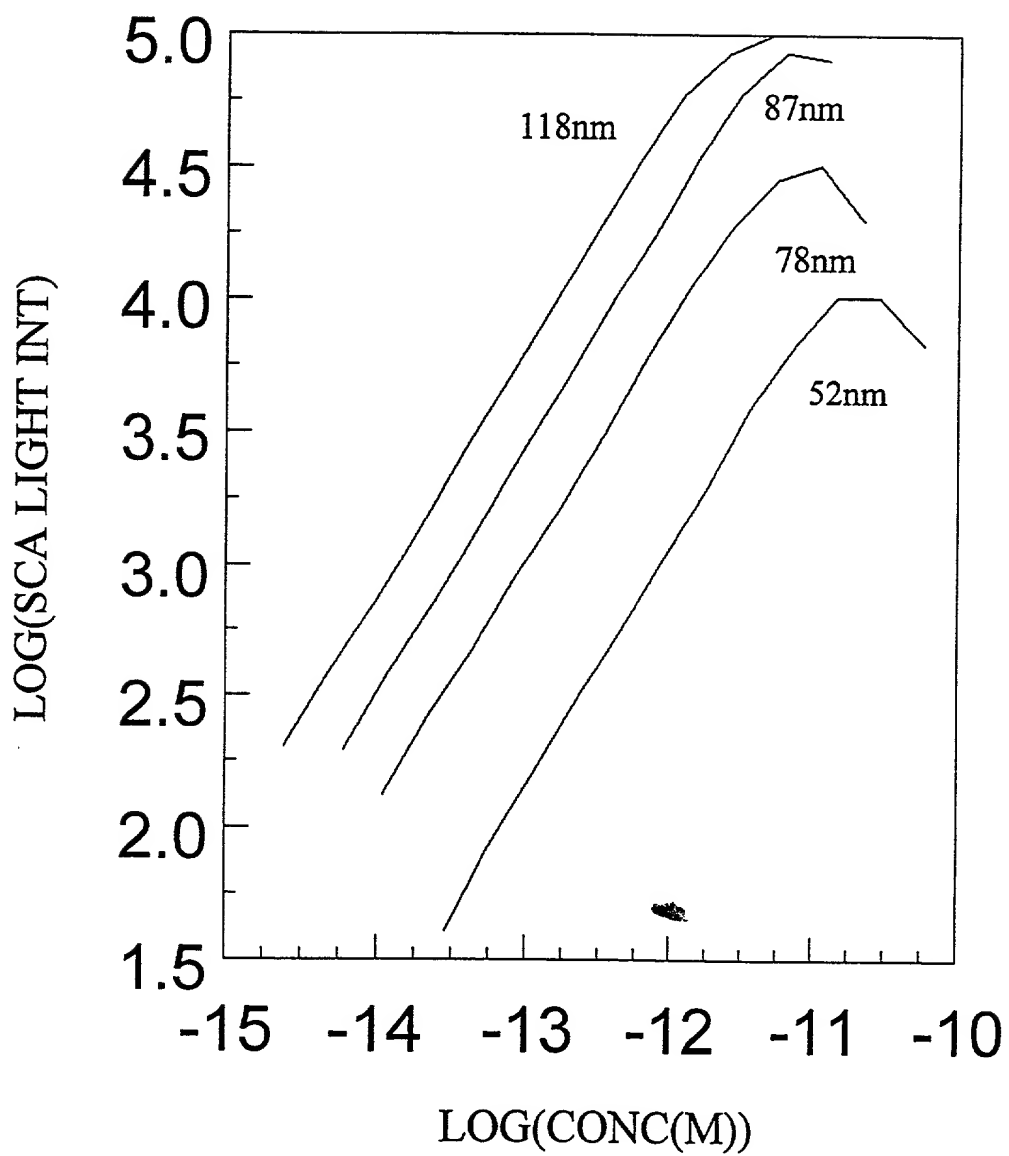


FIGURE 31

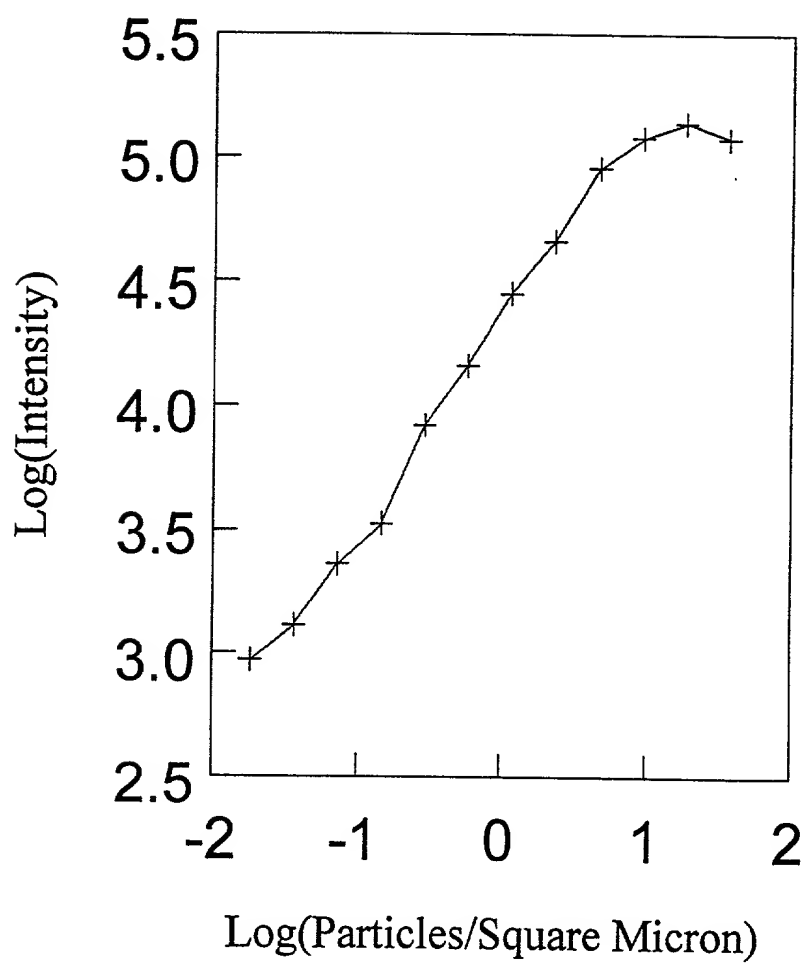


FIGURE 32

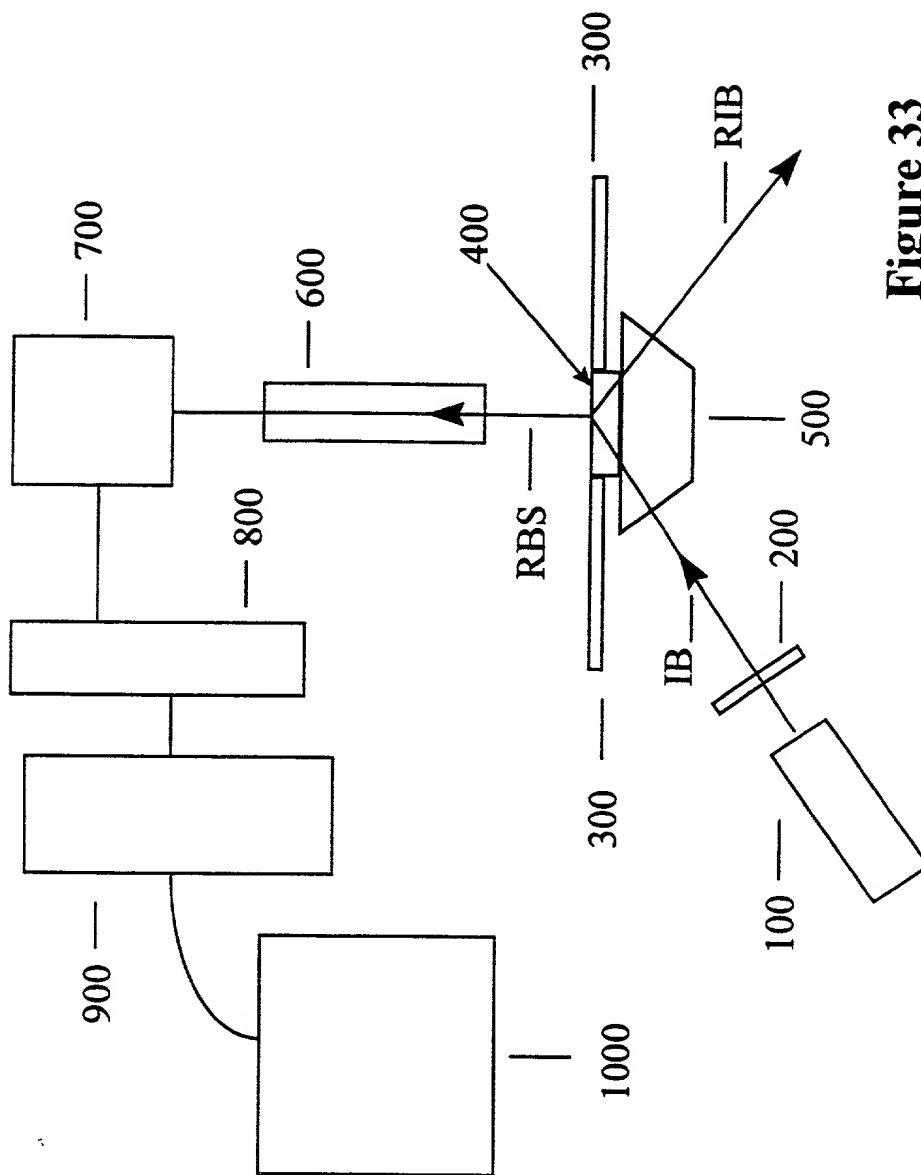


Figure 33